



Use of duplex mutation primers for real-time PCR quantification of hepatitis C virus RNA in serum

Qian-Feng Xia^{1,2}, Yang-An Wen¹, Ping Liu¹, Pu Li¹, Jin-Bo Liu¹, Xi Qin², Shi-Yun Qian², Zhi-Guang Tu^{1*}

¹ The Key Laboratory of Laboratory Medical Diagnostics, Ministry of Education, the Faculty of Laboratory Medicine, Chongqing Medical University, Chongqing, China

² The Faculty of Laboratory Medicine and Tropical Medicine, Hainan Medical College, Haikou, China

ARTICLE INFO

Article Type:
Original Article

Article history:
Received: 06 Dec 2010
Revised: 24 Mar 2011
Accepted: 01 Apr 2011

Keywords:
HCV
Quantification
PCR
Duplex mutation primers
Hepatitis

ABSTRACT

Background: The duplex mutation primers offer many advantages over other multi-labeled probes for real-time detection of amplification products.

Objectives: To develop and validate a novel real-time PCR for quantification of HCV RNA based on the duplex mutation primers technology.

Materials and Methods: The duplex mutation primers were selected in the highly conservative 5' non-coding region (5'NCR) of the HCV RNA. The assay was validated with the Viral Quality Control panel, which also includes Chinese HCV RNA standards.

Results: The detection limit was 57 IU/mL, and a good linear correlation in the range of 102-108 IU/mL was revealed ($r^2 = 0.999$) with the novel method. This assay has a dynamic range of at least 8 log₁₀ without the need for specimen dilution, good clinical intra- and inter-run precision, and excellent correlation with a commercially available assay ($r^2 = 0.95$).

Conclusions: The high sensitivity, wide linear range, and good reproducibility, combined with low cost, make this novel quantitative HCV real-time PCR assay particularly well suited for application to clinical and epidemiological studies.

© 2011 Kowsar M.P.Co. All rights reserved.

► Implication for health policy/practice/research/medical education:

This novel HCV diagnostic assay is recommended to all clinicians involved in diagnosis and treatment of patients with HCV infection. We also suggest reader's attention in the field of real-time PCR and liver infection diseases to the conclusion of this article.

► Please cite this paper as:

Xia QF, Wen YA, Liu P, Li P, Liu JB, Qin X, et al. Use of duplex mutation primers for real-time PCR quantification of hepatitis C virus RNA in serum. *Hepat Mon.* 2011;11(7):519-24.

1. Background

Quantitative hepatitis C virus (HCV) RNA determinations are currently the standard of care for diagnosis of acute and chronic HCV infections and monitoring for therapeutic efficacy. Several home-made and commercial real-time PCR assays have been used

to quantify the level of HCV RNA in serum samples (1-3). The nonspecific dsDNA binding dyes methods are prone to "false positives" in that undesired dsDNA such as primer dimers and other spurious amplicons can bind dyes to produce fluorescence (4). Well-known specific multi-labeled FRET probes examples include TaqMan (5), molecular beacons (6), scorpion primers (7), and amplifluor (8). The synthesis and purification of these multi-labeled probes are often either trivial or expensive relative to the pair of fluorophore and the quencher in the same oligonucleotide. Although hybridization probes (9), displacing probes (10) and Q-PNA primers (11) have

* Corresponding author at: Zhi-Guang Tu, The Key Laboratory of Laboratory Medical Diagnostics, Ministry of Education, the Faculty of Laboratory Medicine, Chongqing Medical University, 400016, Chongqing, China. Tel: +86-2368485759, Fax: +86-2368485005.

E-mail: zhiguangtu@sina.com

some advantages over multi-labeled probes. However, both hybridization probes and displacing probes need the phosphatation to block the amplification, are not real single-labeled probes and the costs are increased. We reported a new method based on duplex mutation primers, in which a primer with a fluorophore is attached at its 5'-end, and a complementary oligonucleotide with a single-base mismatched is labeled by a quencher at 3'-end (12). Incorporation of the fluorophore primer into a double stranded amplicon causes the physical separation of the fluorophore and quencher moieties, and produces an increase of the fluorescence signal, which is the direct indicator of the template concentration. The duplex mutation primers are much more specific than double-strand DNA dyes like SYBR Green I, etc. Unlike other probes (5-8), duplex mutation primers do not require the double labeled synthesis of fluorophore and quencher on the same molecule, which makes the synthesis of the FRET probe less costly and design more convenient.

2. Objectives

The purpose of this study was to report the development of a quantitative real-time PCR HCV RNA assay using duplex mutation primers technology. We evaluated the sensitivity, specificity and efficacy of this assay and its usefulness for the diagnosis of HCV infection. The correlation between results with this assay and with the TaqMan assay was investigated.

3. Materials and Methods

3.1. Patient samples

The clinical samples included 92 sera collected from patients with an acute or chronic HCV infection. To test for specificity, we used samples anonymously obtained from each of the following groups: apparently healthy volunteers of our hospital (n = 60), HBV-monoinfected patients (n = 45), and HAV-monoinfected patients (n = 5). All healthy volunteers had normal serum ALT levels and were negative for antibodies to HCV by ELISA. For all samples, sera was separated from whole blood, aliquoted, and stored at -20°C until it was further processed.

3.2. Viruses for analytical studies

The Chinese National standard for HCV, which has an assigned concentration of 1.25×10^6 IU/mL, was serially diluted in negative human plasma to a final concentration ranging from 1×10^6 to 1×10^2 IU/mL, and were used as reference standards for each real-time PCR run. Analytical verification studies (measurable range, LOD, and precision) were performed with a commercial panel of clinical specimens containing HCV Gt 1a, Gt 2b, and Gt 3a viruses (DaAn, Ltd. Guangzhou, China). For a standardized evaluation, we obtained a Chinese National reference viral quality control (VQC) plasma preparation panel containing well-characterized HCV RNA levels. These samples were tested extensively and

contain HCV RNA levels ranging from no HCV RNA to 10^7 HCV molecules per mL.

3.3. Nucleic acid extraction

Total RNA was extracted from 200 μ L of serum with a Trizol kit (Invitrogen, USA) according to the manufacturer's instructions. After the extraction by the Trizol kit, the total amount of extracted nucleic acids was solved in 100 μ L.

3.4. Reverse transcription

A total volume of 25 μ L of reverse transcription reaction mixture was prepared as follow: 1 μ L of random primers (0.2 μ g/ μ L, Promega, USA) was added to 5 μ L of extracted HCV RNA. The mixture was denatured at 70°C for 5 minutes and cooled on ice immediately. Then 5 μ L of 5 \times reverse transcription buffer, 0.75 μ L of RNasin (40 U/ μ L, Promega, USA), 1 μ L of M-MLV reverse transcriptase (200 U/ μ L, Promega, USA), 1.25 μ L of dNTP (10 mM, Promega, USA) and 11 μ L of RNase-free water were added into the reaction tube. The tube was flicked gently and incubated for 60 minutes at 37°C. The reaction was terminated at 95°C for 5 minutes. Reverse transcription products (cDNA) were frozen at -20°C until further use. The presence of HCV cDNA in these samples was then analyzed with commercial TaqMan kit (Da'an Ltd., Guangzhou, China) and our method.

3.5. Preparation of duplex mutation primers

The fluorophore primers (5'-FAM-CGACACTCCACCATAGATCAC-3') and the reverse primers (5'-AGGCTGCACGACACTCATAAC-3') were used to amplify a 94-bp fragment in the highly conservative 5' non-coding region (5'NCR) of the HCV RNA. The fluorophore primers were quenched by partly complementary oligonucleotides (5'-GTGATCTATGGCGGAGTGTCG-Dabcyl-3') of a single-base mismatched labeled with a quencher at 3'-end. All of the primers were selected using the primer premier 5.0 software and were synthesized, purified and labeled by Takara Ltd. Dalian, China.

Table 1. Limit of the HCV RNA real-time PCR assay

Concentration, IU/mL	positive, % (positive/total replicates, No.)
400	100 (8/8)
200	100 (8/8)
100	100 (8/8)
50	87.5 (7/8)
25	50 (4/8)
12.5	37.5 (3/8)
6.3	12.5 (1/8)
3.1	0
1.6	0

Table 2. Study of intra and inter-run variability of the HCV RNA real-time PCR assay to determine its precision

	HCV RNA, IU/mL					Mean	SD	CV, %
	1	2	3	4	5			
Intra-run								
1	2.14×10 ²	2.36×10 ²	2.24×10 ²	2.01×10 ²	1.95×10 ²	2.14×10 ²	1.67×10 ¹	7.80
2	1.39×10 ³	1.21×10 ³	1.24×10 ³	1.31×10 ³	1.19×10 ³	1.27×10 ³	8.2×10 ¹	6.46
3	5.17×10 ⁴	5.36×10 ⁴	5.25×10 ⁴	5.19×10 ⁴	5.12×10 ⁴	5.22×10 ⁴	9.2×10 ²	1.76
4	7.45×10 ⁷	7.37×10 ⁷	7.39×10 ⁷	7.41×10 ⁷	7.31×10 ⁷	7.39×10 ⁷	5.2×10 ⁵	0.70
Control	N ^a	N	N	N	N	-	-	-
Inter-run								
1	2.44×10 ²	2.31×10 ²	2.12×10 ²	2.19×10 ²	1.85×10 ²	2.18×10 ²	2.22×10 ¹	10.18
2	1.39×10 ³	1.32×10 ³	1.20×10 ³	1.27×10 ³	1.15×10 ³	1.27×10 ³	9.50×10 ¹	7.48
3	5.17×10 ⁴	5.24×10 ⁴	5.09×10 ⁴	5.31×10 ⁴	5.37×10 ⁴	5.24×10 ⁴	1.11×10 ³	2.12
4	7.51×10 ⁷	7.37×10 ⁷	7.30×10 ⁷	7.21×10 ⁷	7.47×10 ⁷	7.37×10 ⁷	1.23×10 ⁵	1.67
Control	N	N	N	N	N	-	-	-

^aN: negative

3.6. Real-time PCR system

Real-time PCR was performed with a Rotor-Gene 3000 (Corbett Robotics, Australia). The total volume of the real-time PCR was 20 µL containing 5 µL of cDNA, 4 µL duplex mutation primers (2.0 µM of the fluorophore primer, 2.0 µM of the quencher strand), 4 µL reverse primer (2.0 µM), 2.5 µL each dNTP (1.6 mM, Takara Ltd. Dalian, China), 2 µL 10× buffer, 0.2 µL of Taq polymerase (5 U, Takara Ltd. Dalian, China) and 1 µL MgCl₂ (25 mM, Takara Ltd. Dalian, China), adding distilled water to 20 µL. The cycling parameters were an initial denaturation at 94 °C for 5 min, 40 cycles of 93 °C for 15 s, and 48 °C for 15 s. The signal detection was performed at 48 °C during each cycle. To quantify the starting template in samples, the samples were run in along with a standard curve generated from 10-fold serially diluted standard serum of a known concentration.

3.7. Lower limit of detection

To test for the lower limit of detection, the stock of the commercial panel of clinical specimen was diluted with sterile water to 400, 200, 100, 50, 25, 12.5, 6.3, 3.1, and 1.6 IU/mL. Eight replicates of each dilution and two negative controls were then tested by our method.

3.8. Linearity

To test the linearity of the quantitative PCR, the stock of the HCV reference standard at a concentration of 1.25×10⁶ IU/mL, was diluted stepwise (1:10), and four to six replicates were tested per dilution. Furthermore, a high concentration plasma sample (as measured by the HCV Diagnostic kit) from a patient was diluted stepwise (1:10), and two replicates per dilution were tested.

3.9. Precision


To test the inter-run precision, four samples of HCV RNA from patients with low, medium and high levels of viremia as well as one sample from healthy volunteers were aliquoted and stored at -20 °C before use. These five samples were repeatedly assayed five times in five independent experiments. The results of quantitation, along with standard deviations and coefficients of variation (CVs), intra-run precision were determined by measuring the amount of HCV RNA in the 5 samples mentioned above within one PCR run.

3.10. Correlation between the novel PCR assay and a commercially assay

The HCV RNA real-time PCR assay was compared with a commercially available TaqMan assay (Diagnostic kit for HCV, DaAn, China) to determine its usefulness for a clinical virology laboratory. A total of 202 serum specimens were tested by both methods. Samples were not tested simultaneously on both platforms but were first tested by the commercially available assay and then frozen at -20 °C until RNA extraction and the novel PCR testing. Specimens throughout the range of quantification were chosen for analysis. Data were logarithmically transformed before analysis.

3.11. Data analysis

Reproducibility was estimated by computing CVs. The difference of the quantitative results between the commercial TaqMan kit and the developed method was assessed by the paired-sample Student's t test or the Sign test when the results were not distributed normally. Probit statistics was performed to determine the limit of detection of our HCV real-time PCR assay. $P < 0.05$ were considered statistically significant.

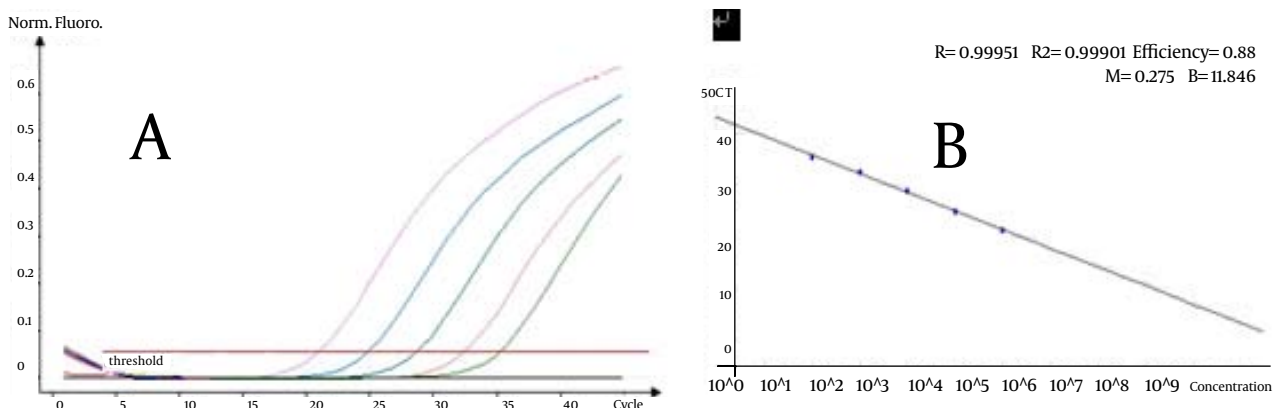Figure 1. Fluorescent curves of the standard dilution series

From the left to the right, these nine fluorescent curves from 10^6 to 10^2 IU/mL are shown; and the negative control is represented by the horizontal black curve (A). Standard curve used to calculate the concentration of HCV RNA in unknown samples. The linear regression coefficient is close to 1 (B).

4. Results

4.1. Real-time PCR detection

The results of real-time PCR analysis of the single copy conservative sequence in HCV genome as a function of template copy number using our primers are shown in Figure 1. A Chinese National standard for HCV dilution series of 10^2 – 10^6 IU/mL was amplified in each PCR run. The cycle threshold (Ct) was automatically set by the instrument software. The calibration curve of Ct vs. template copy number showed linear regression analysis of the best-fit line yielded a good coefficient of determination (r^2) of 0.999 (Figure 1). Analysis of reaction products by electrophoresis revealed that the correct size of the reactions produced amplicons.

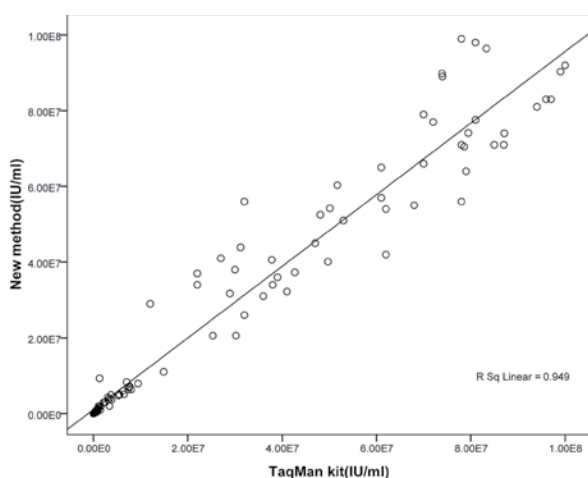


Figure 2. Graph showing correlation of the HCV real-time PCR assay results with the new method results for 92 HCV-positive clinical specimens (numerical values are not listed). There was excellent correlation ($r = 0.95$) between the two assays for all samples.

4.2. Limit of detection

The samples yielded positive results in 100% of replicate reactions at concentrations greater than or equal to 100 IU/mL. Below the concentration, the detection failure rate increased as the concentration decreased (Table 1). A clinical sample was quantified by serially diluting the stock solution, performing eight amplifications with the novel method, and calculating the concentration from the fraction of negative reactions by application of Poisson's law. A detailed probit analysis indicated that the limit of detection (the concentration at which 95% or more of the replicates tested gave a positive response) of the test was 57 IU/mL.

4.3. Linearity

Linearity was confirmed using a patient sample with high levels of HCV RNA. After various dilutions, the nucleic acid was extracted and the HCV RNA was quantified. Linearity was observed from 10^2 up to 10^8 IU/mL in the sample.

4.4. Precision

The inter- and intra-run variability were tested (see Materials and Methods); the results are shown in Table 2.

4.5. Specificity

To determine the specificity of the real-time PCR detection assay, we used 110 samples anonymously obtained from each of the following groups: apparently healthy volunteers of our hospital ($n = 60$), HBV-monoinfected patients ($n = 45$), and HAV-monoinfected patients ($n = 5$). None of the samples showed false-

positive reactions in duplicate.

4.6. Comparison between two different quantification assays

The presence or quantity of HCV RNA in the sera of the 92 HCV patients was determined by our method and commercial TaqMan kit separately. There was no significant difference among the tested results with two methods in 92 HCV hepatitis patients ($P = 0.723$). A significant positive linear correlation was found ($r^2 = 0.95$, Figure 2).

5. Discussion

Methods for HCV RNA quantitation must be specific, sensitive, reproducible, and accurate. Analysis of large number of samples requires a rapid and manageable protocol that minimizes as much as possible post-PCR manipulations. Endpoint PCR-based techniques for HCV RNA have shown a limited dynamic range, usually within 4 logs, affecting the quantification of moderate to high levels of viremia (13). Real-time PCR is designed to quantify nucleic acids in the exponential phase of the reaction, allowing for a more reliable and precise quantification over a much wider dynamic range. Quantitative tests of HCV RNA levels in serum are currently the standard of care for the diagnosis of acute and chronic HCV infections and monitoring for therapeutic efficacy (14). In this study, we described the development and validation of a novel quantitative real-time PCR assay that showed good performance characteristics in terms of the limit of detection, linearity, reproducibility, and specificity. This assay has good clinical sensitivity at 57 IU/mL using an initial sample volume of only 200 μ L, at least an 8 log₁₀ linear dynamic range without the need for specimen dilution. This linearity was well in line with the linearity of other assays performed on the Cobas TaqMan HCV platform (15). The low variability of this assay makes a twofold decrease or increase in the serum HCV RNA level already significant. The mandatory requirement of 100% specificity was achieved, as none of the controls, including healthy donors and patients infected with HBV or HAV, was tested positive HCV RNA. Nevertheless, the number of control samples need to be increased to further confirm these findings. The high reproducibility and linearity of the assay described proved to be comparable with one commercially available assay. Our method has several advantages over the other multi-labeled probes methods; higher specificity: the primers are duplex form and cannot hybridize with each other at lower temperature than their melting temperature that minimizes non-specific annealing in the course of amplification. Higher sensitivity: after primer-target hybridization, the distance between the fluorophore and the quencher changes from close proximity to totally free separation. This property endows them with

stronger signal than other internal FRET probes. Higher cost/efficiency: single-labeled oligonucleotides structure makes the synthesis less costly and design more convenient than multi-labeled probes. In conclusion, a duplex mutation primers real-time PCR system with high cost/efficiency, rapid, sensitive and high specificity has been developed for the quantitative detection of HCV RNA. The assay is suitable to be used for both clinical and epidemiological studies.

Financial support

None declared.

Conflict of interest

None declared.

Acknowledgments

This work was supported by grant HjKj200524 and Hj2010-20 from the Education Bureau of Hainan province.

References

1. Forman MS, Valsamakis A. Verification of an assay for quantification of hepatitis C virus RNA by use of an analyte-specific reagent and two different extraction methods. *J Clin Microbiol.* 2004;**42**(8):3581-8.
2. Jongerius JM, Sjerps M, Cuijpers HT, van Drimmelen HA, van der Poel CL, Reesink HW, et al. Validation of the NucliSens Extractor combined with the AmpliScreen HIV version 1.5 and HCV version 2.0 test for application in NAT minipool screening. *Transfusion.* 2002;**42**(6):792-7.
3. Konnick EQ, Williams SM, Ashwood ER, Hillyard DR. Evaluation of the COBAS Hepatitis C Virus (HCV) TaqMan analyte-specific reagent assay and comparison to the COBAS AmpliCor HCV Monitor V2.0 and Versant HCV bDNA 3.0 assays. *J Clin Microbiol.* 2005;**43**(5):2133-40.
4. Wittwer CT, Herrmann MG, Moss AA, Rasmussen RP. Continuous fluorescence monitoring of rapid cycle DNA amplification. *Biotechniques.* 1997;**22**(1):130-1, 4-8.
5. Holland PM, Abramson RD, Watson R, Gelfand DH. Detection of specific polymerase chain reaction product by utilizing the 5'→3' exonuclease activity of Thermus aquaticus DNA polymerase. *Proc Natl Acad Sci U S A.* 1991;**88**(16):7276-80.
6. Tyagi S, Kramer FR. Molecular beacons: probes that fluoresce upon hybridization. *Nat Biotechnol.* 1996;**14**(3):303-8.
7. Xia QF, Xu SX, Wang DS, Wen YA, Qin X, Qian SY, et al. Development of a novel quantitative real-time assay using duplex scorpion primer for detection of Chlamydia trachomatis. *Exp Mol Pathol.* 2007;**83**(1):119-24.
8. Nazarenko IA, Bhatnagar SK, Hohman RJ. A closed tube format for amplification and detection of DNA based on energy transfer. *Nucleic Acids Res.* 1997;**25**(12):2516-21.
9. Wittwer CT, Ririe KM, Andrew RV, David DA, Gundry RA, Balis UJ. The LightCycler: a microvolume multisample fluorimeter with rapid temperature control. *Biotechniques.* 1997;**22**(1):176-81.
10. Cheng J, Zhang Y, Li Q. Real-time PCR genotyping using displacing probes. *Nucleic Acids Res.* 2004;**32**(7):e61.
11. Fiandaca MJ, Hyldig-Nielsen JJ, Gildea BD, Coull JM. Self-reporting PNA/DNA primers for PCR analysis. *Genome Res.* 2001;**11**(4):609-13.
12. Xia QF, Tu ZG, Liu JB, Qin X, Qian SY, Li P. Detection of PCR products using self-reporting duplex mutation primers. *J Clin*

- Pathol.* 2009;**62**(11):1046-8.
13. Young KK, Archer JJ, Yokosuka O, Omata M, Resnick RM. Detection of hepatitis C virus RNA by a combined reverse transcription PCR assay: comparison with nested amplification and antibody testing. *J Clin Microbiol.* 1995;**33**(3):654-7.
 14. White PA, Pan Y, Freeman AJ, Marinos G, Ffrench RA, Lloyd AR, et al. Quantification of hepatitis C virus in human liver and serum samples by using LightCycler reverse transcriptase PCR. *J Clin Microbiol.* 2002;**40**(11):4346-8.
 15. Sizmann D, Boeck C, Boelter J, Fischer D, Miethke M, Nicolaus S, et al. Fully automated quantification of hepatitis C virus (HCV) RNA in human plasma and human serum by the COBAS AmpliPrep/COBAS TaqMan system. *J Clin Virol.* 2007;**38**(4):326-33.

Copyright of Hepatitis Monthly is the property of Tehran Hepatitis Center and its content may not be copied or emailed to multiple sites or posted to a listserv without the copyright holder's express written permission. However, users may print, download, or email articles for individual use.